

V 2400

The current version of the installation and operating instructions is available in the Download Center:



<http://qr.duerrdental.com/9000-606-97>




Ambient temperature



Upper limit of humidity



Only qualified specialists or employees trained by Dürr Dental are permitted to install, connect and start using the unit.

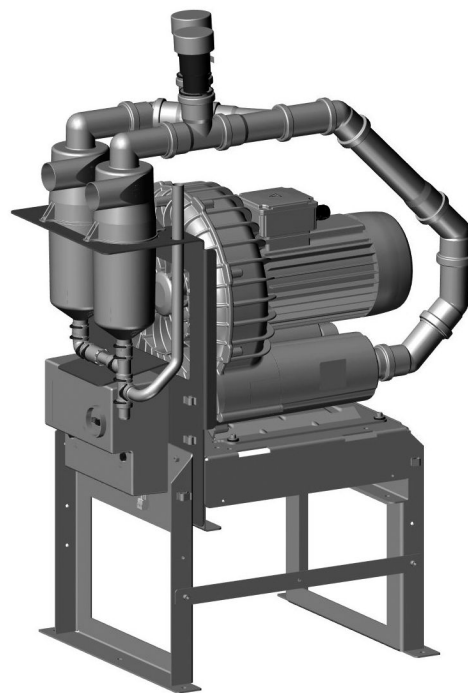


1



► Use advantages and profit with security. Register your product now!


Assembly

1

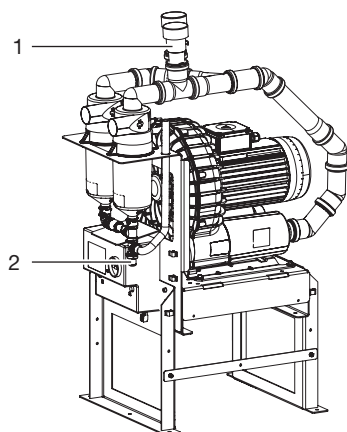


- 1 Auxiliary air valve
- 2 Waste water outlet

2

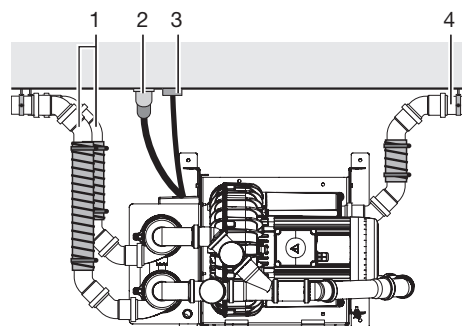

- 1 Suction connections
- 2 Power supply
- 3 Control line
- 4 Exhaust air line

3

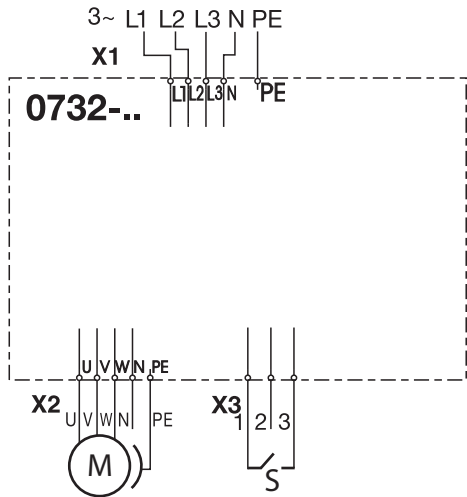


3~

- X1 Mains connection
- X2 Suction unit connection
- X3 Control voltage output, control signal input
- M Suction unit
- S Switching contact to floor connection of the treatment unit

Usage


Disinfection and cleaning

1

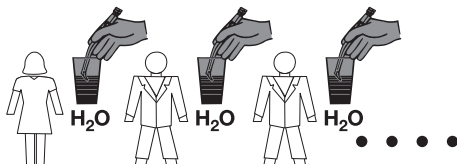


2

1x / Day
in the evenings



1-2x / Week
about noon



3

